

FIG. 1

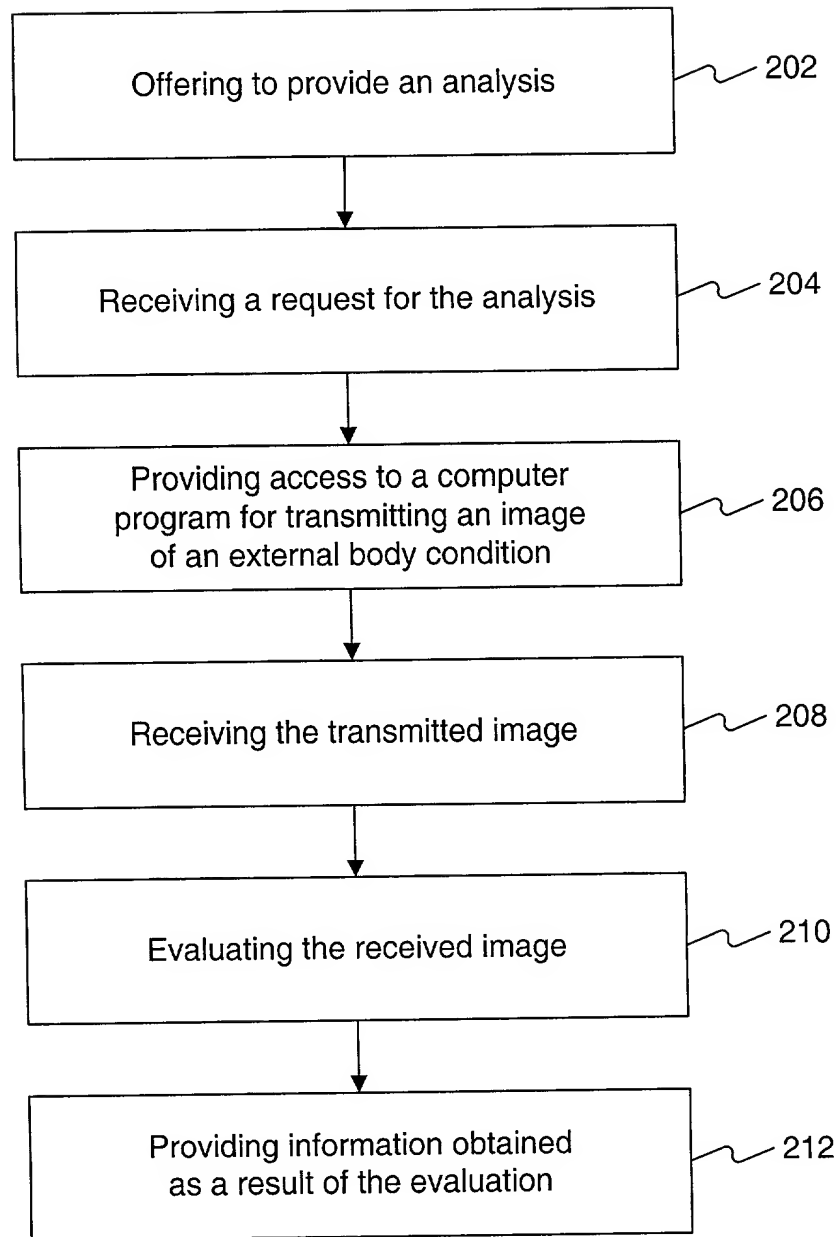


FIG. 2

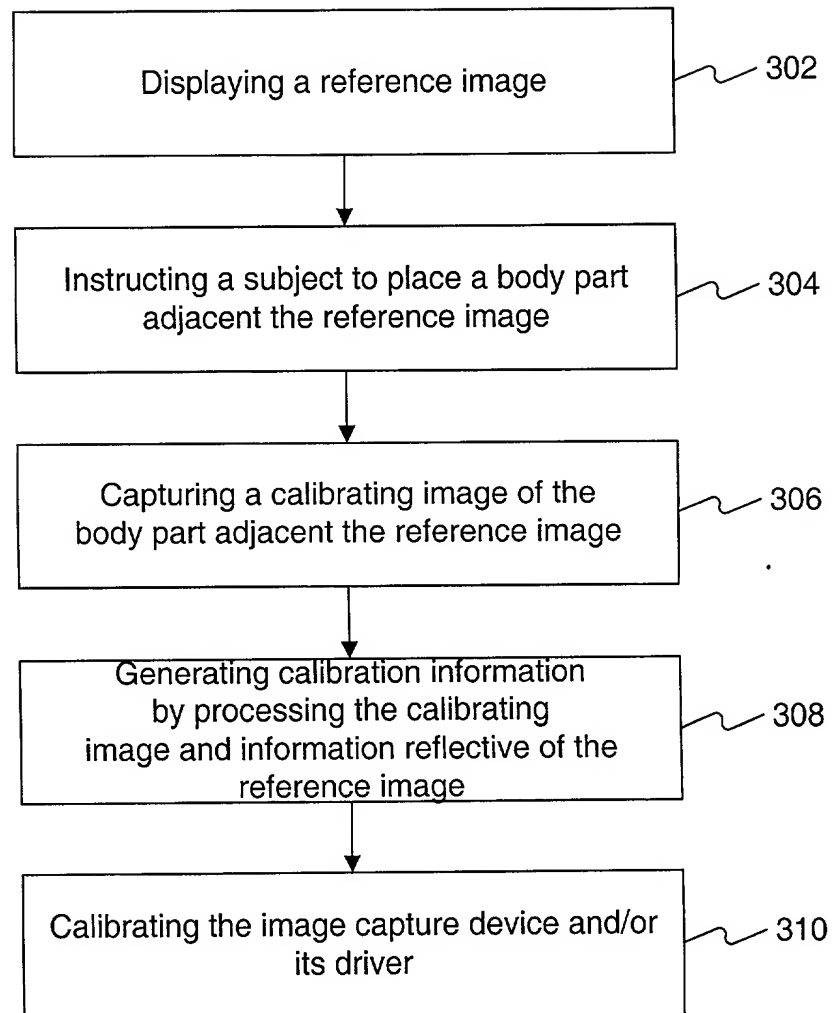


FIG. 3

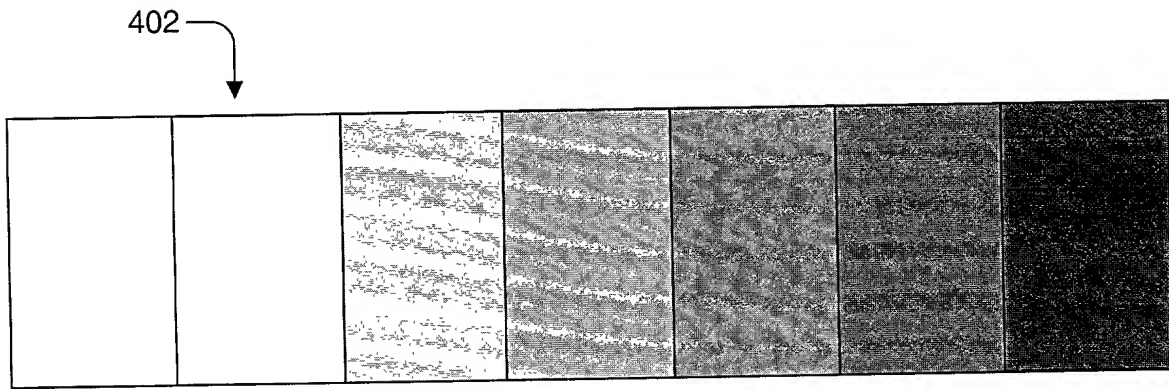


FIG. 4A

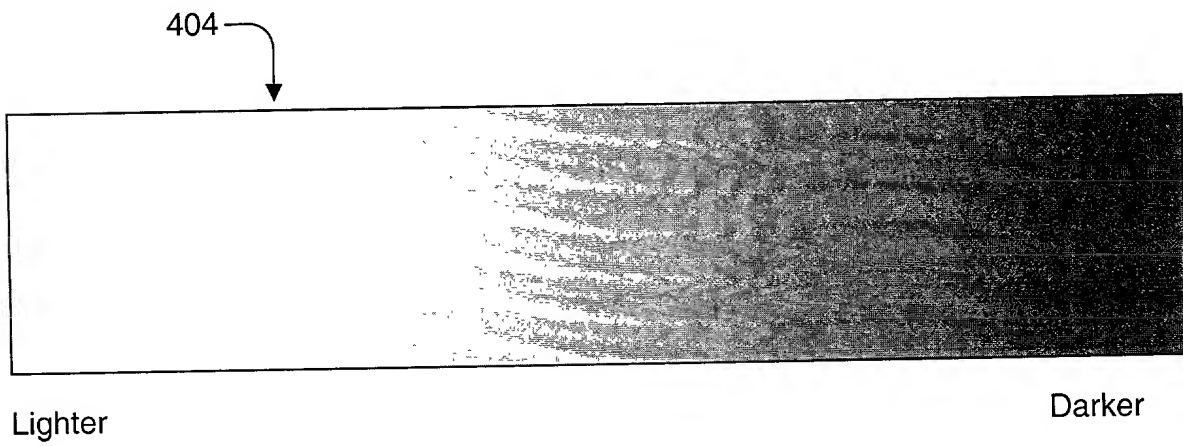


FIG. 4B

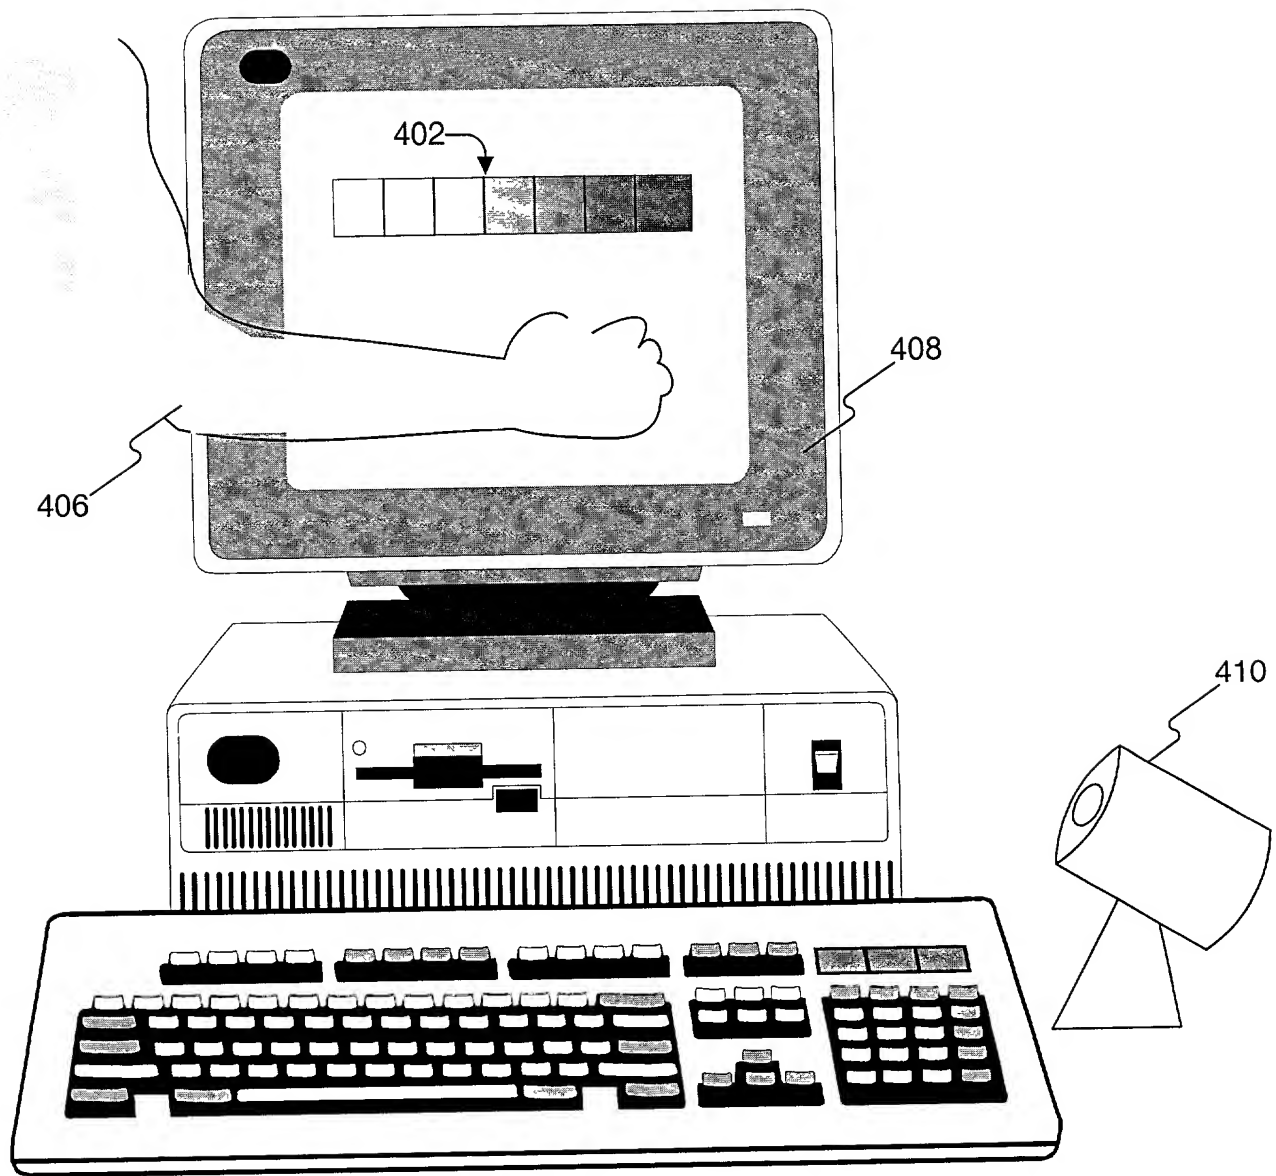


FIG. 4C

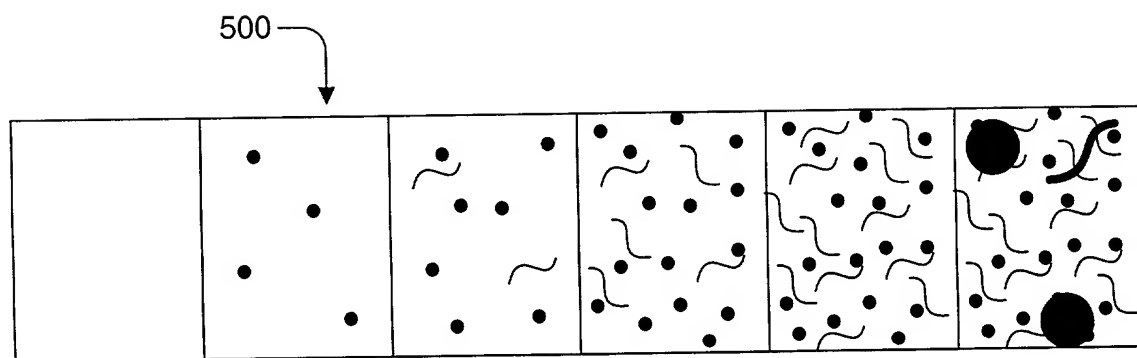


FIG. 5

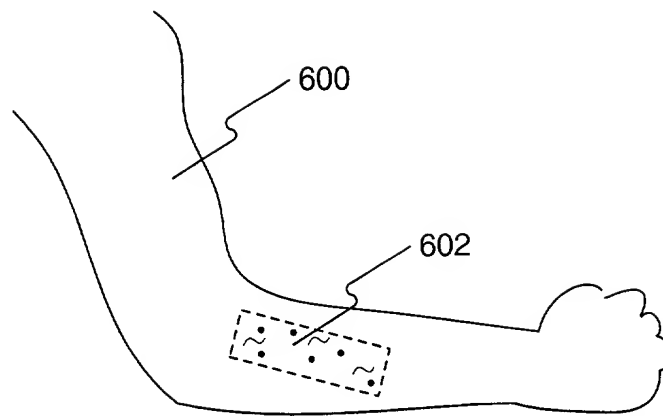


FIG. 6A

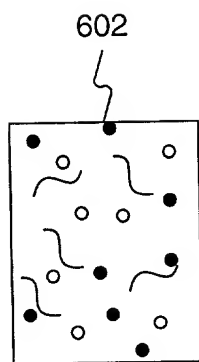


FIG. 6B

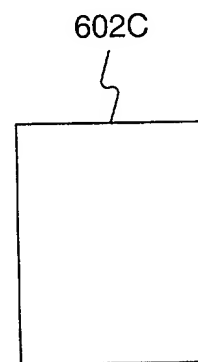


FIG. 6C

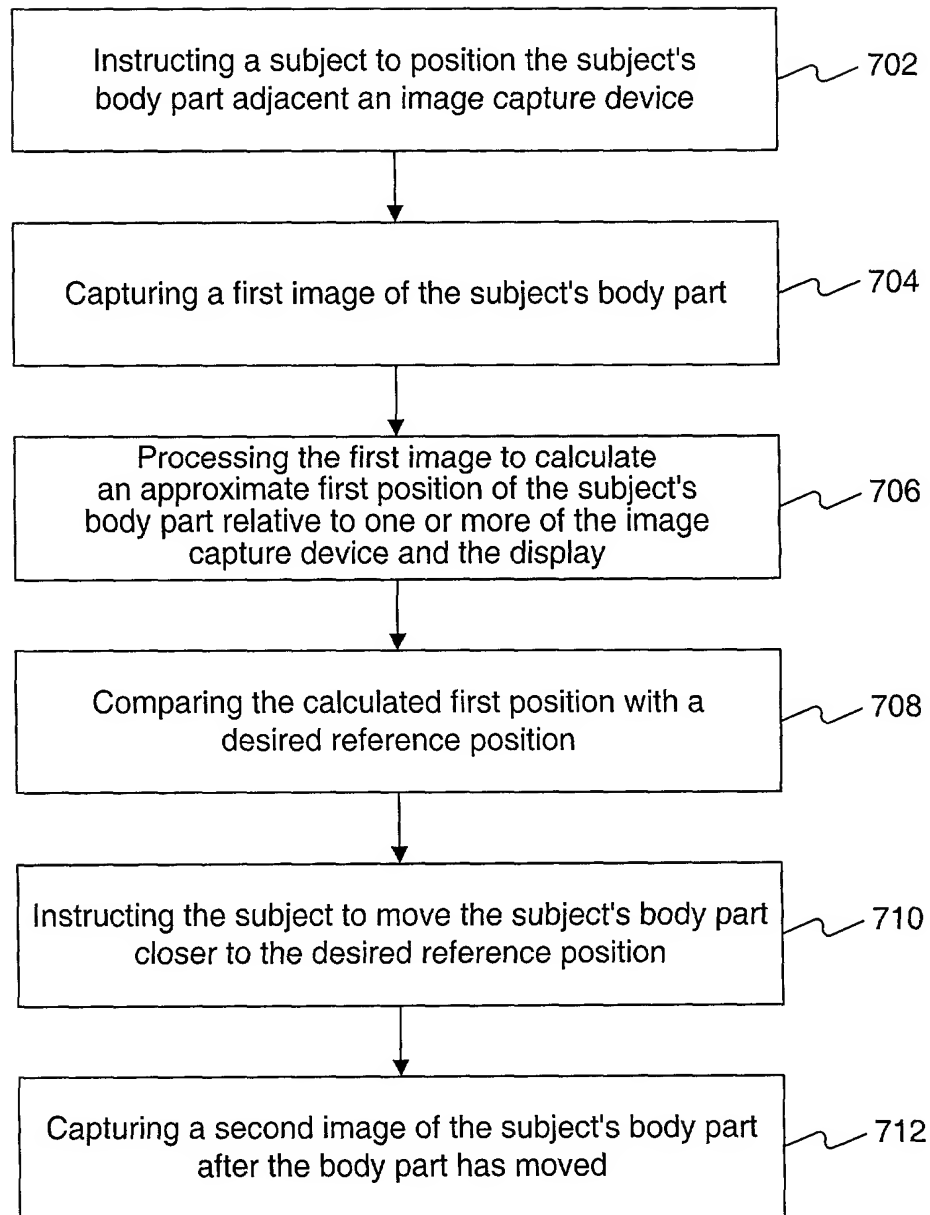


FIG. 7

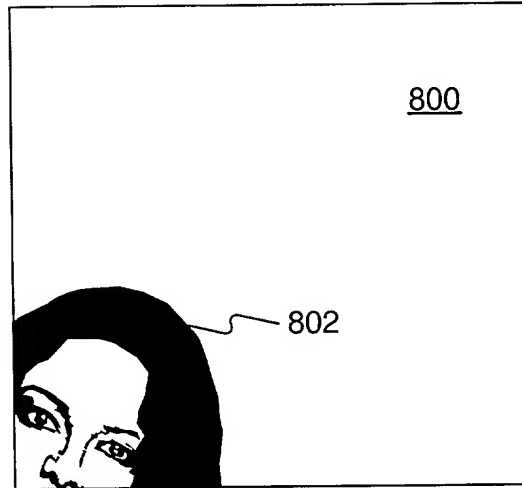


FIG. 8A

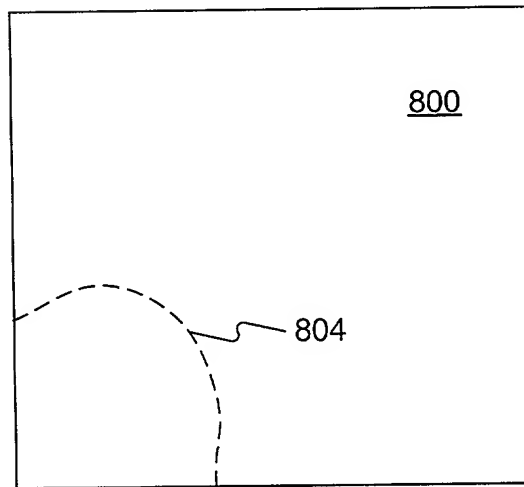


FIG. 8B

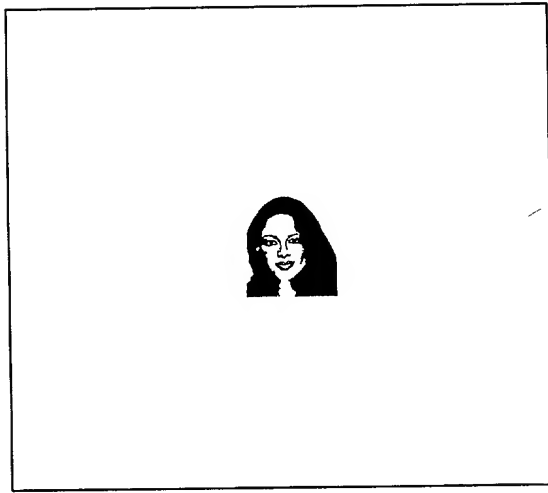


FIG. 9A

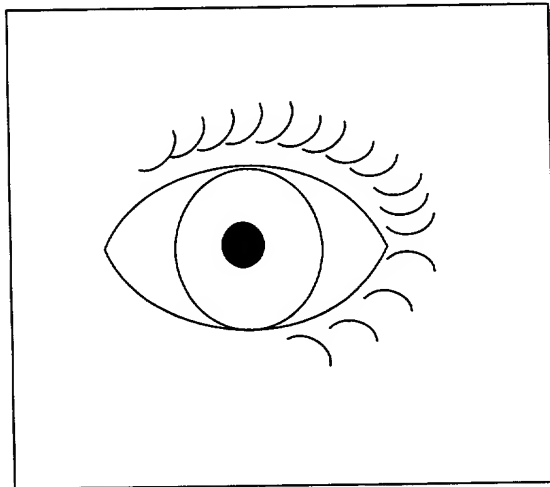


FIG. 9B

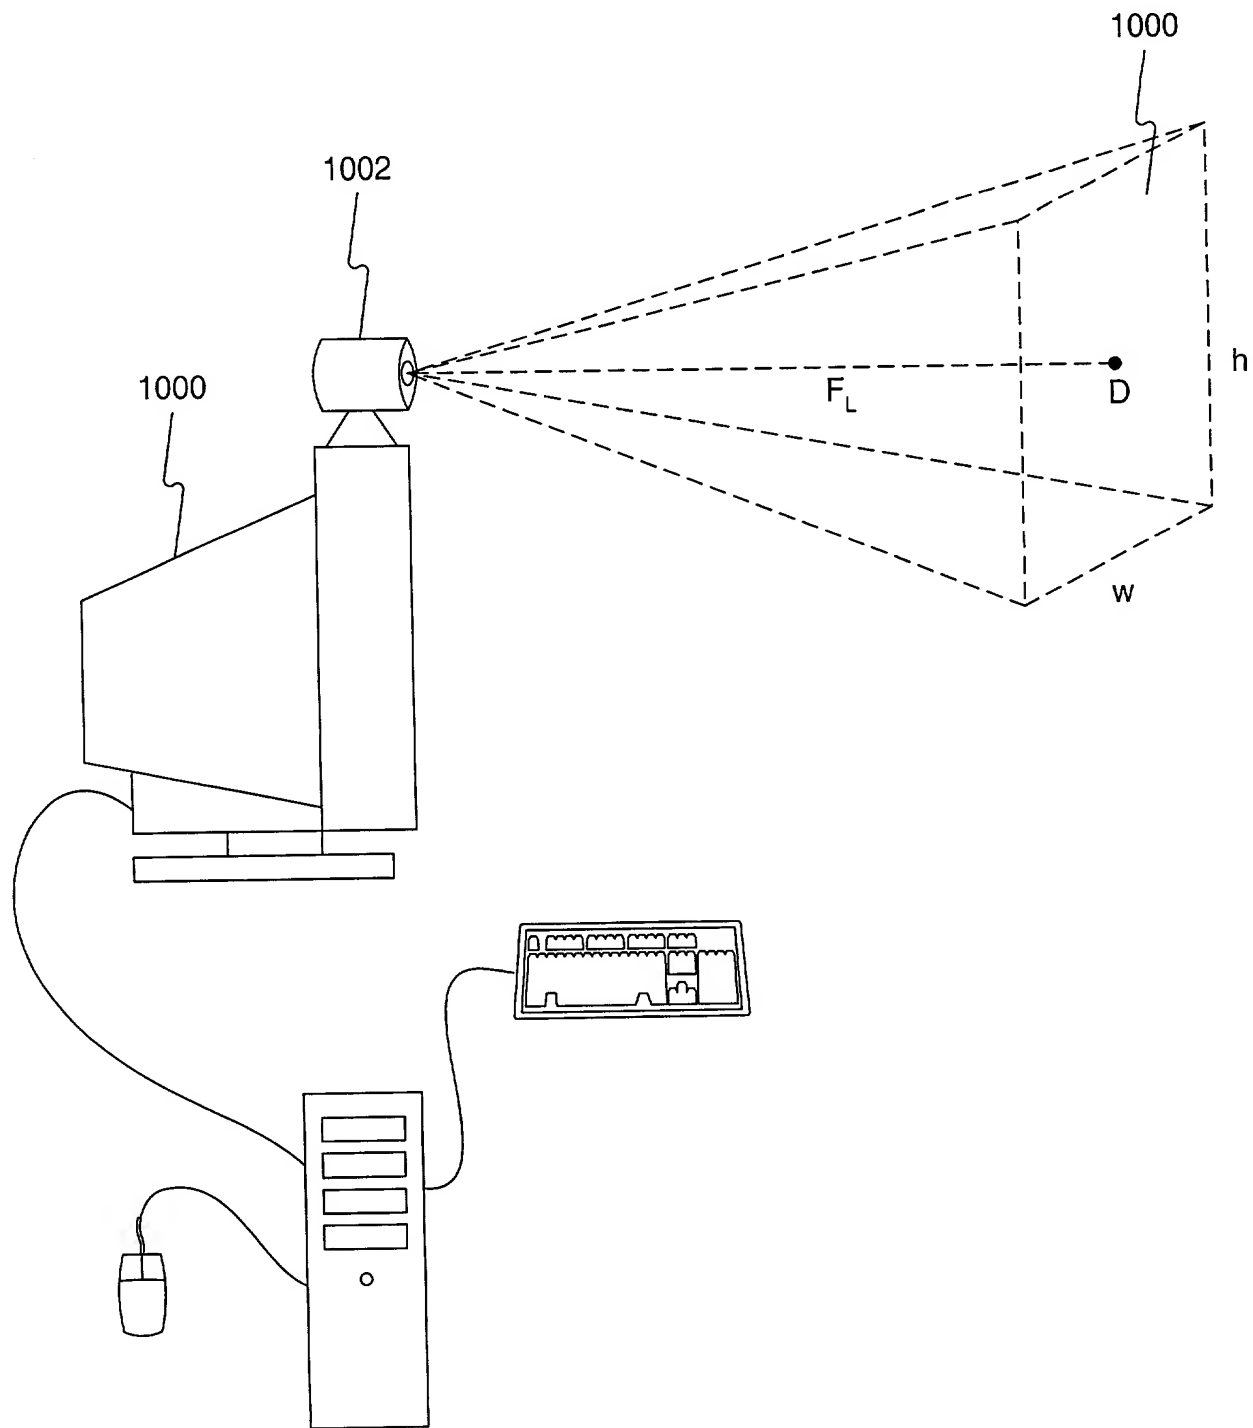


FIG. 10

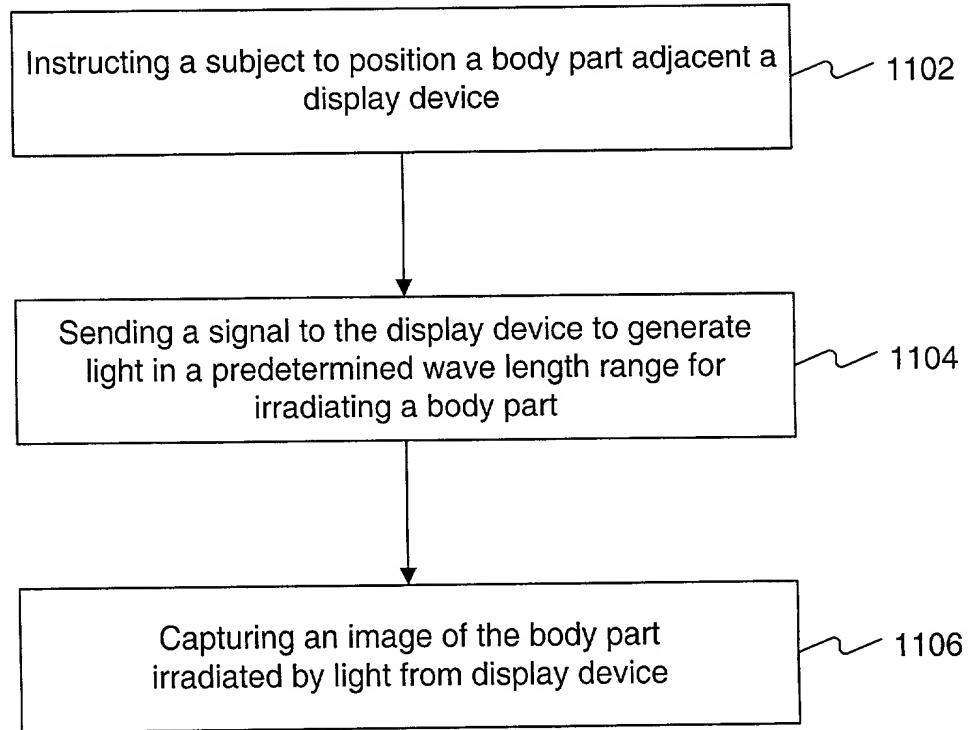


FIG. 11

FIG. 12 is a schematic diagram of a customized diagnostic kit 900. The kit includes a sebutape 902, a d-squame disc 904, a pH indicator 906, a Corneodisque indicator 908, a floppy disk 912, and a camera 910.

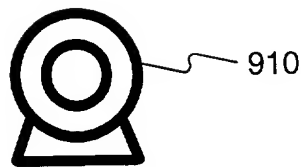
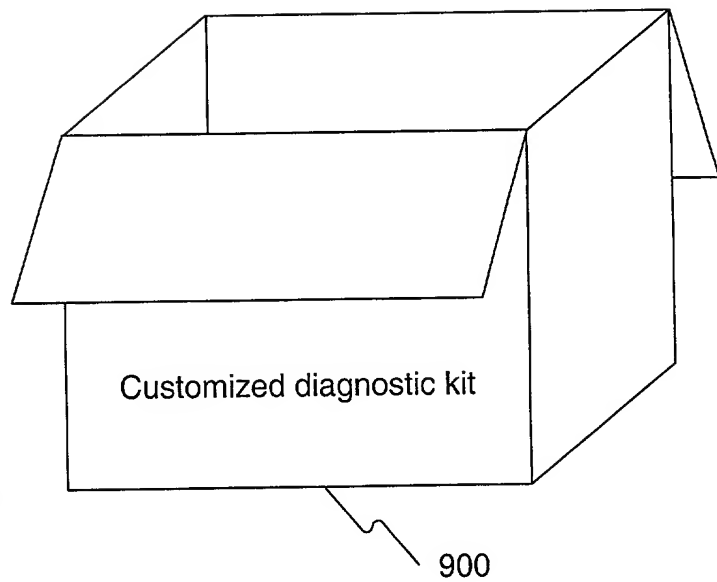
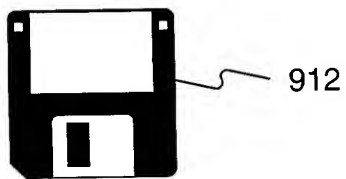

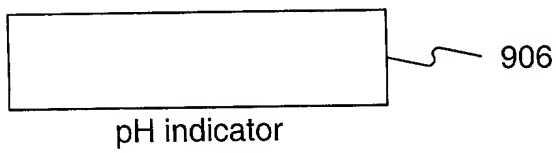
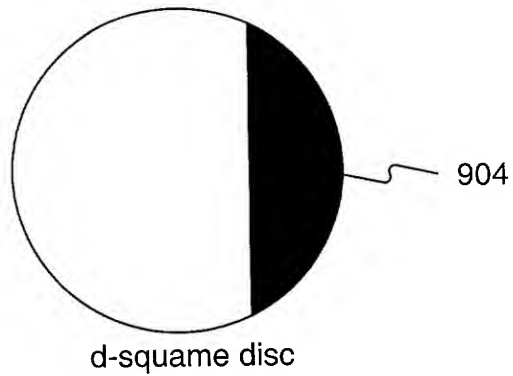
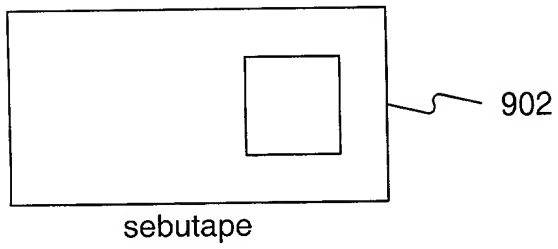


FIG. 12

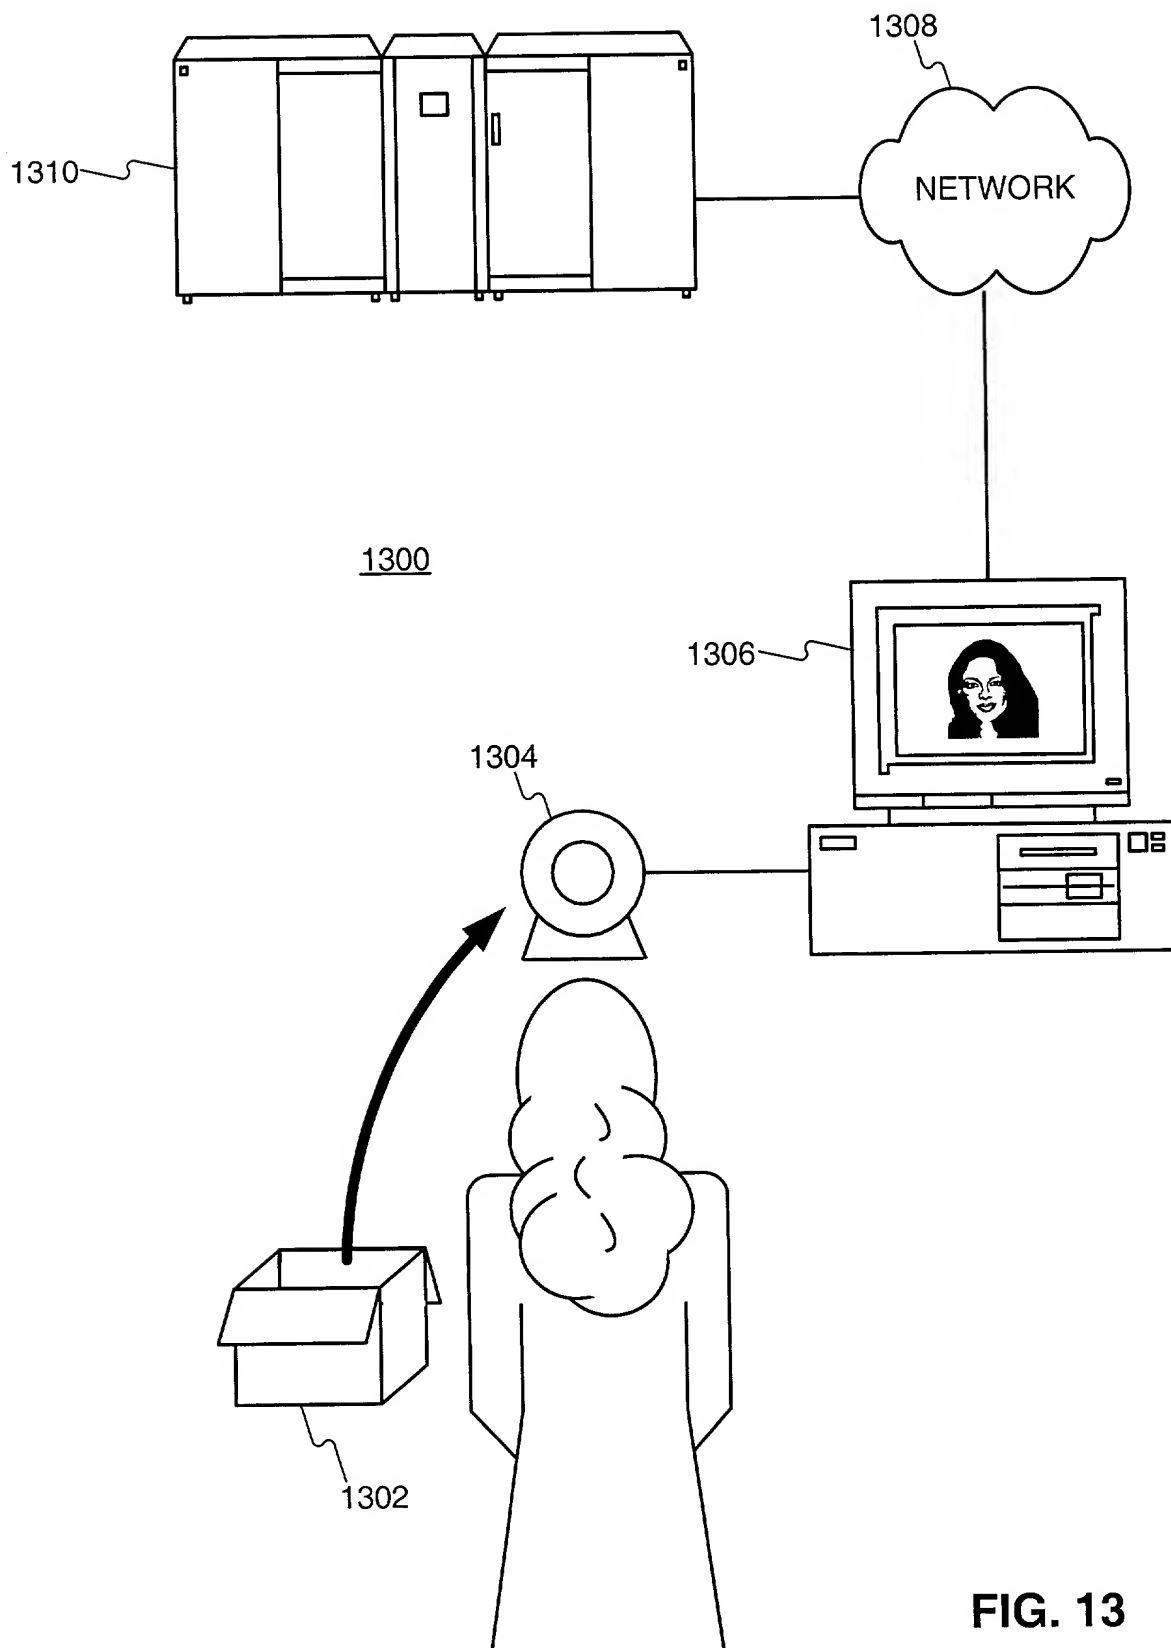


FIG. 13